

FIG.1

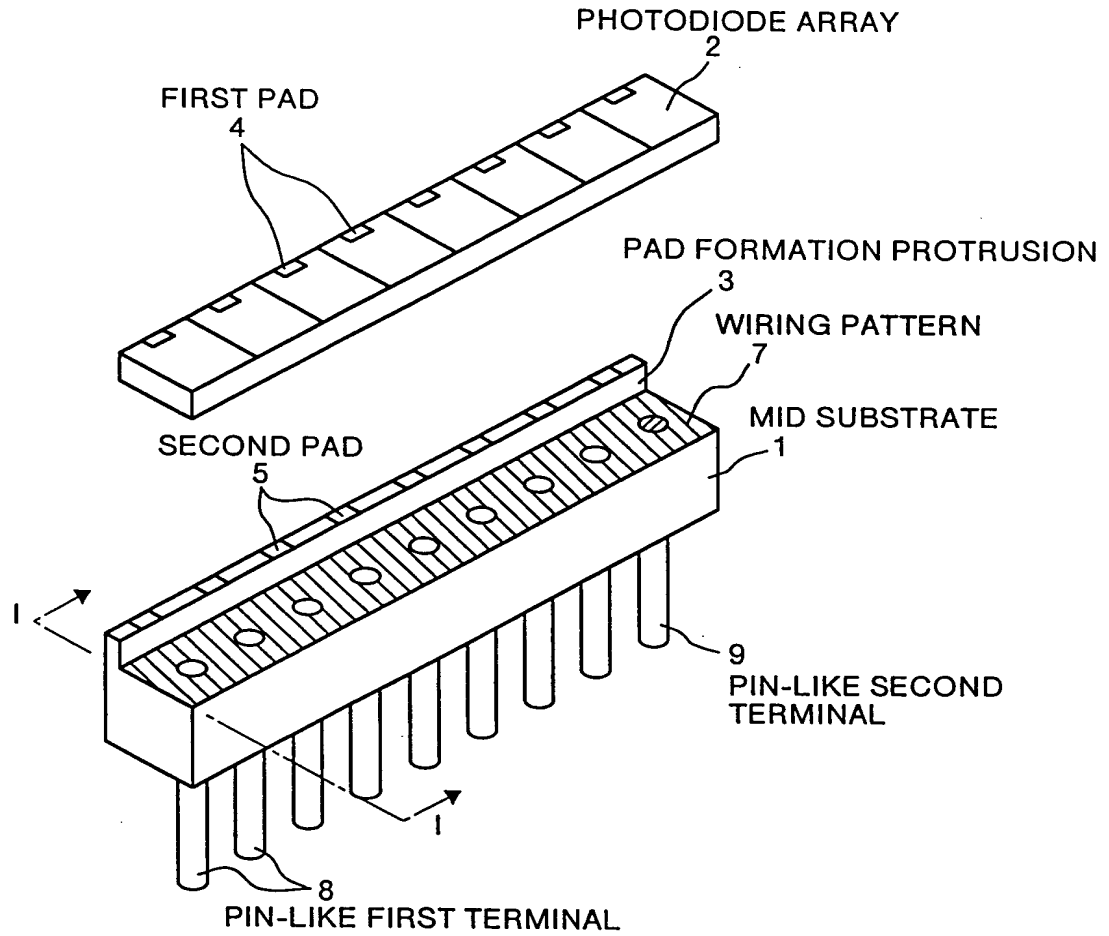


FIG.2

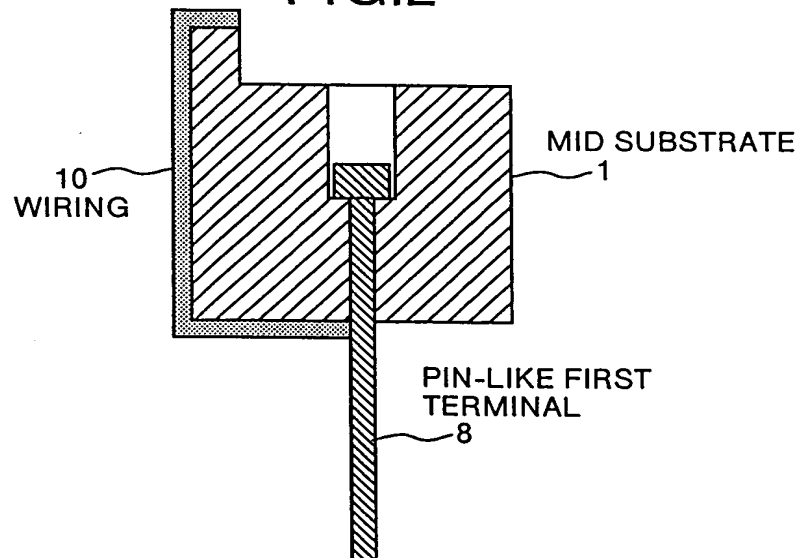


FIG.3A

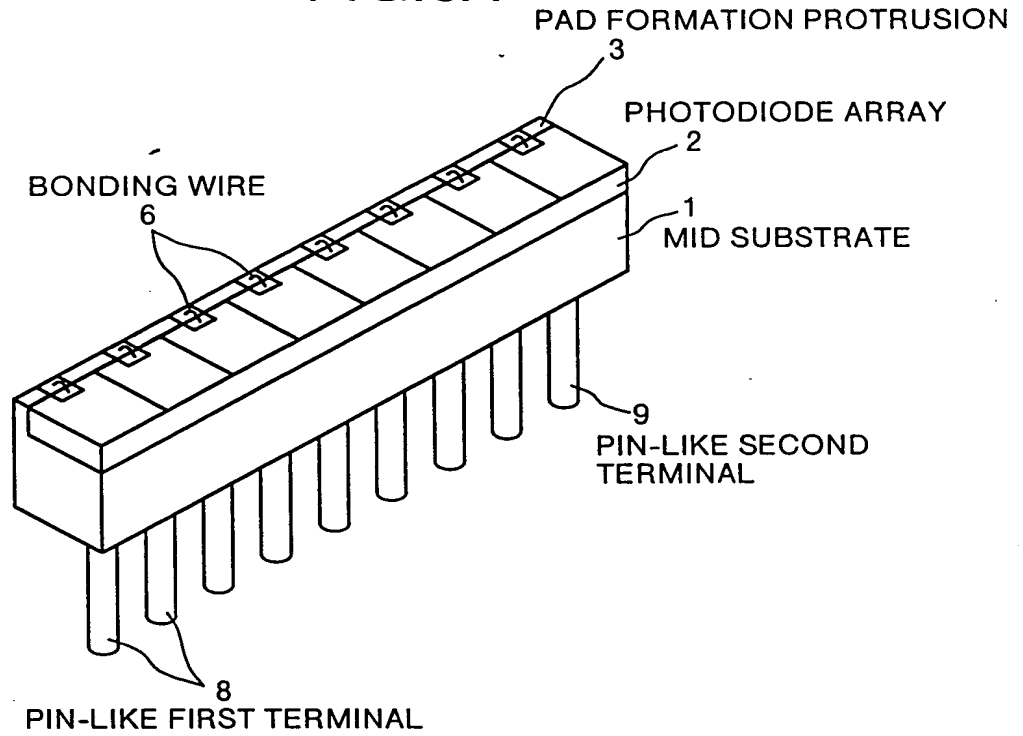


FIG.3B

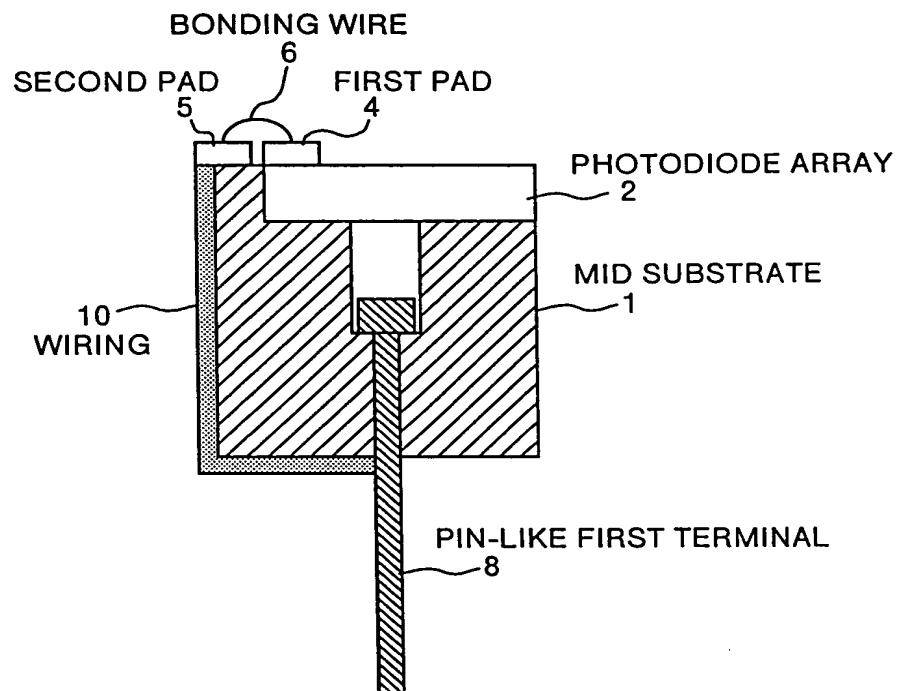


FIG.4

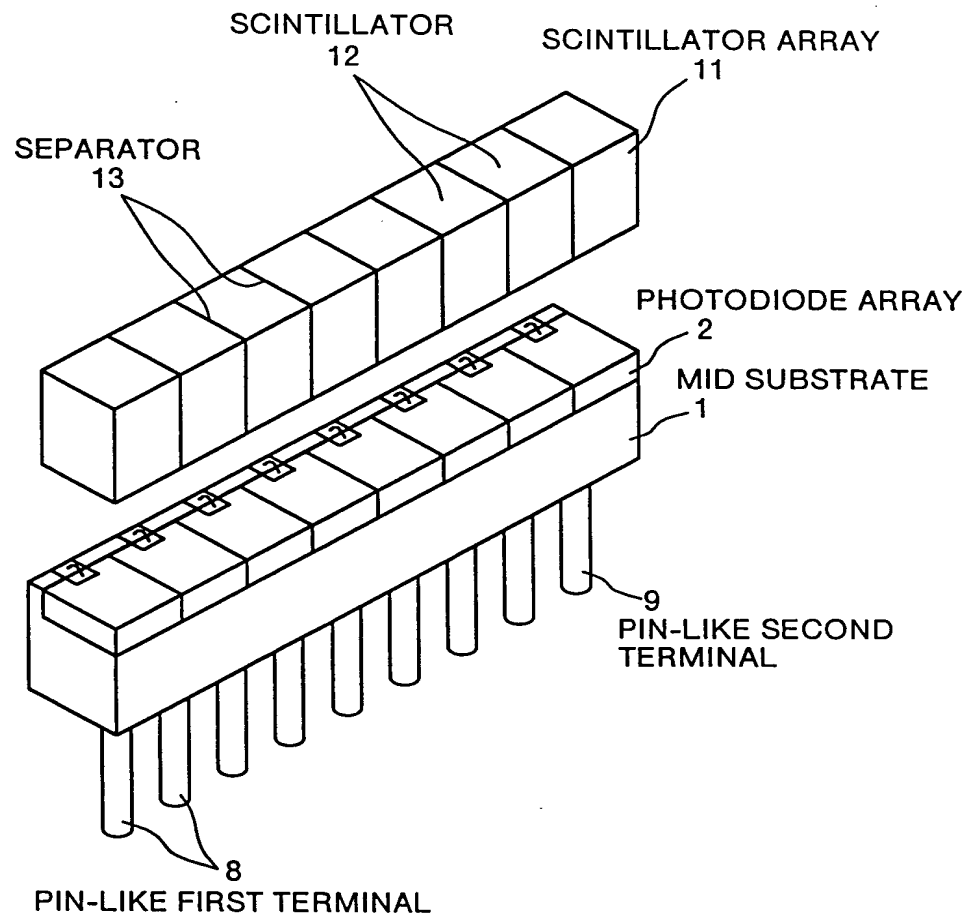


FIG.5

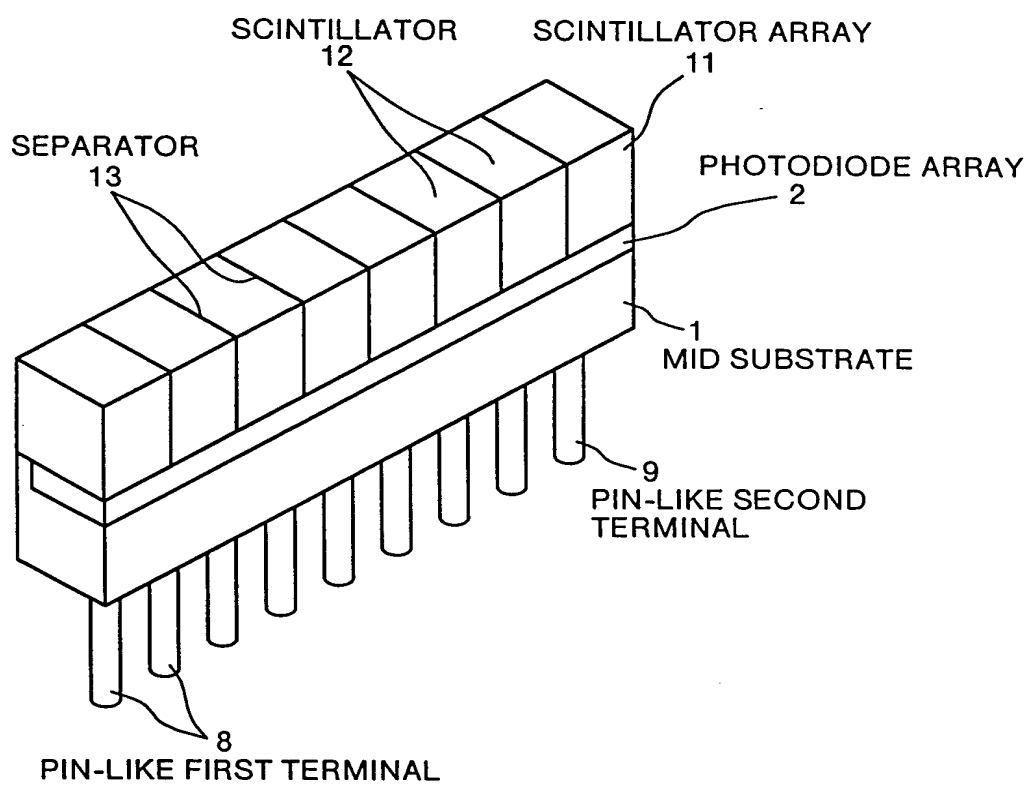


FIG.6

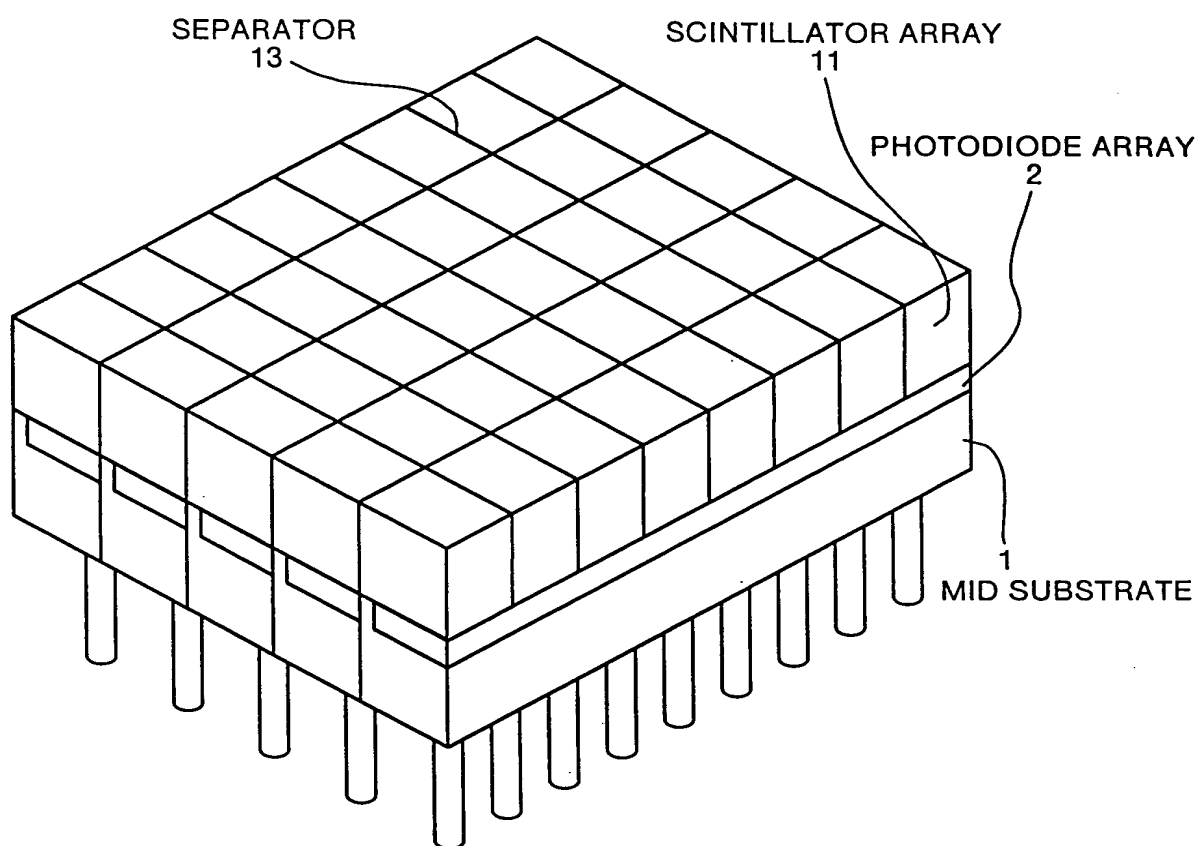


FIG. 7

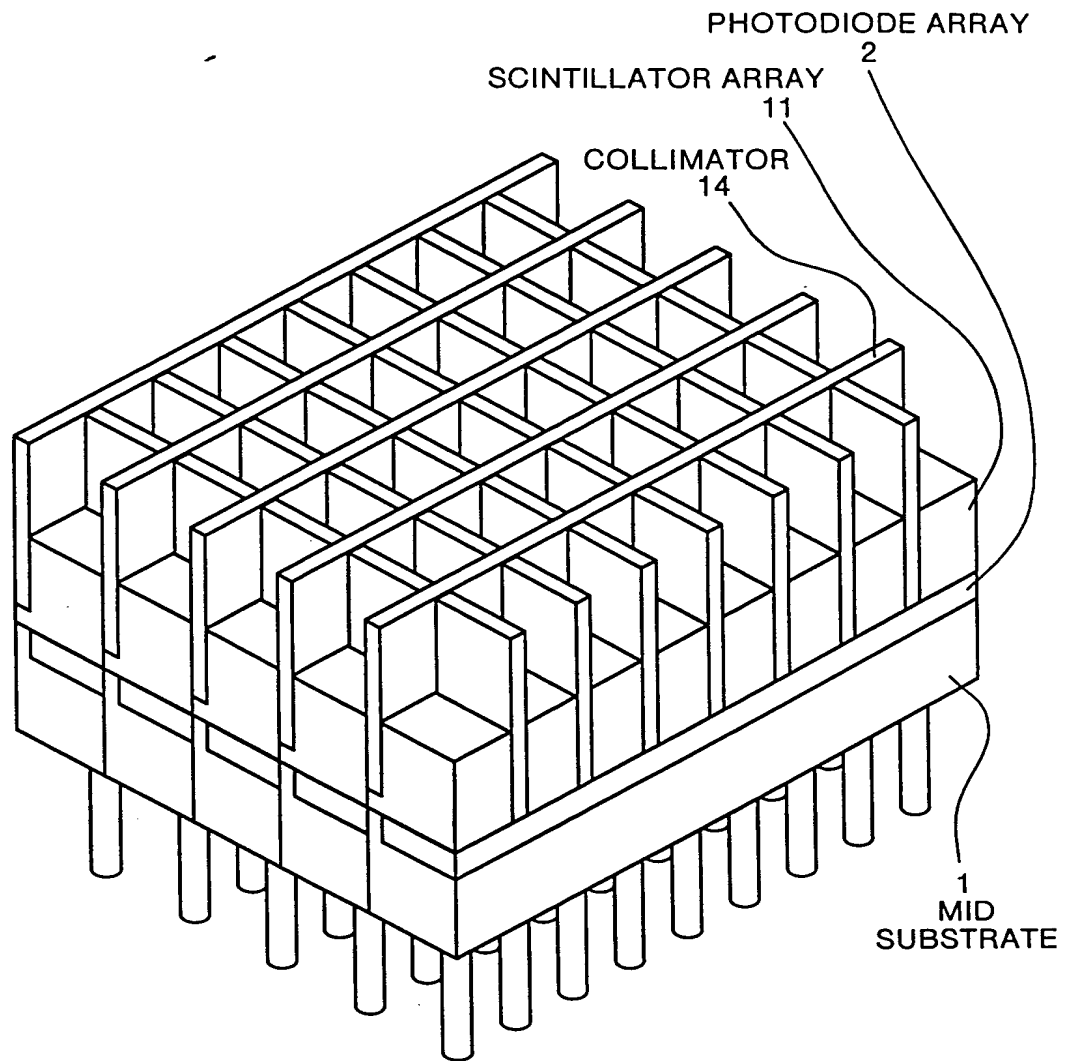


FIG.8A

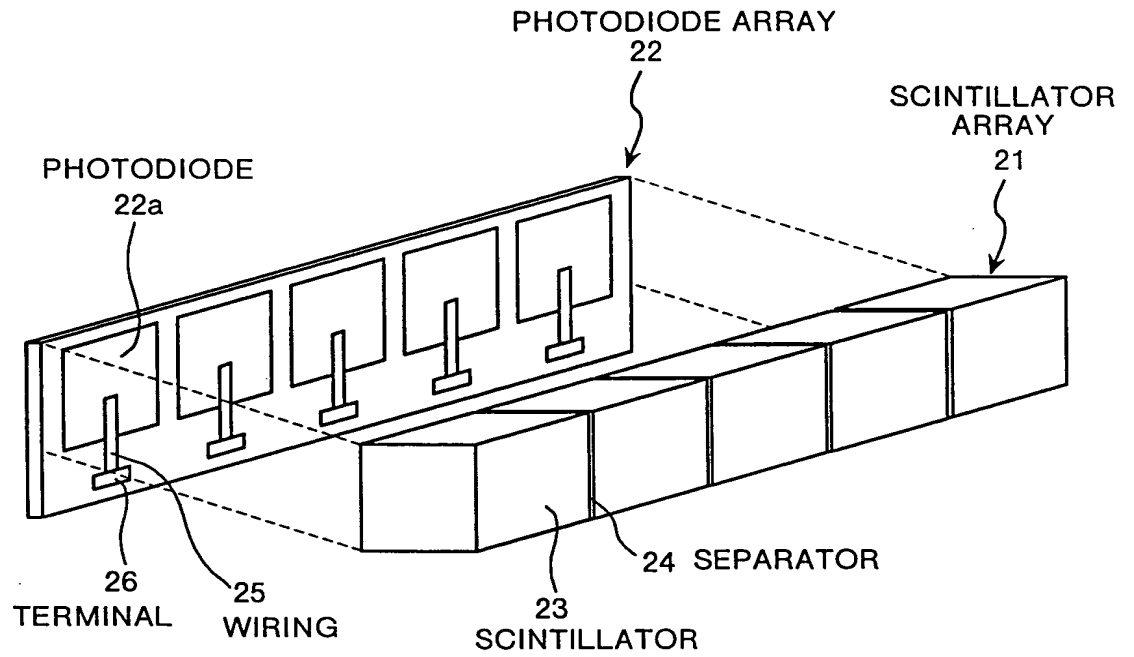


FIG.8B

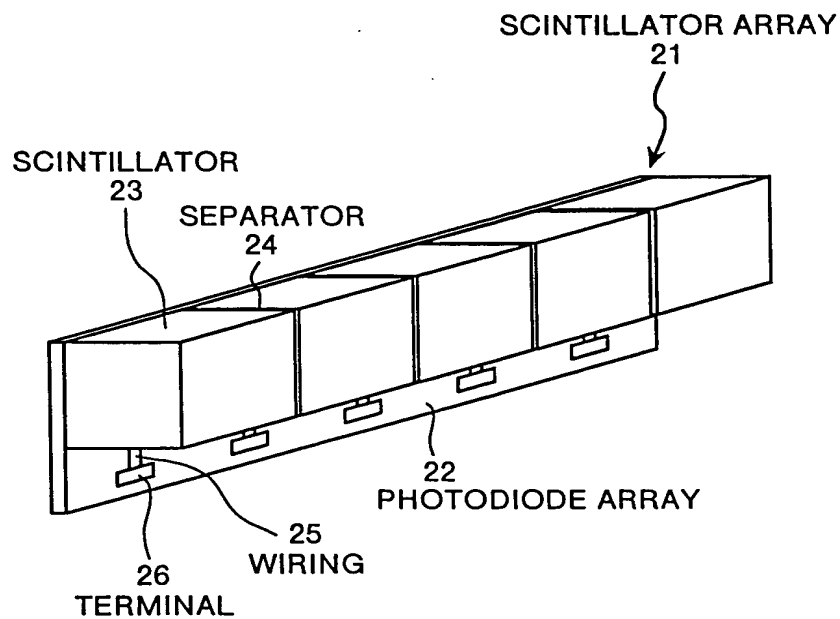


FIG.9

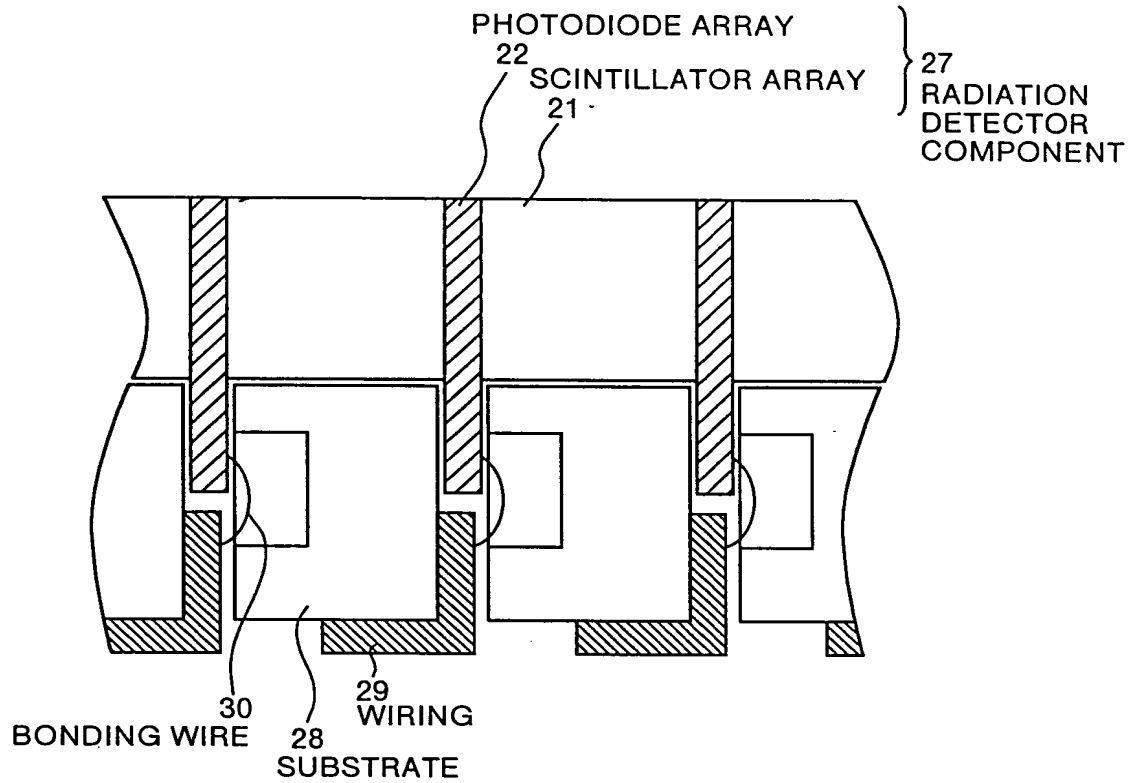


FIG.10

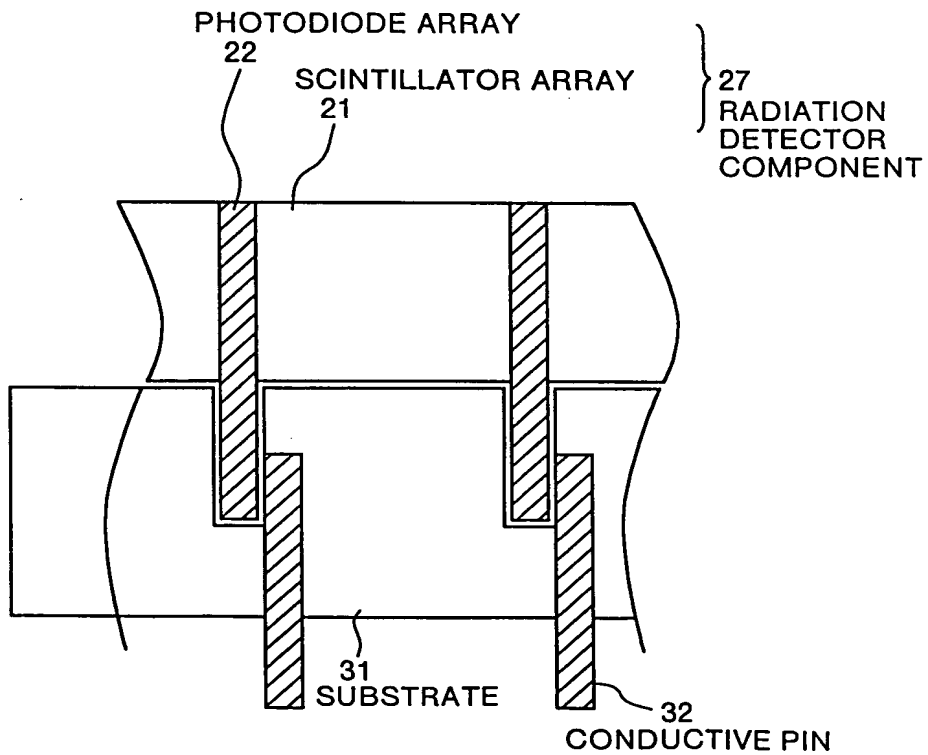




FIG.11

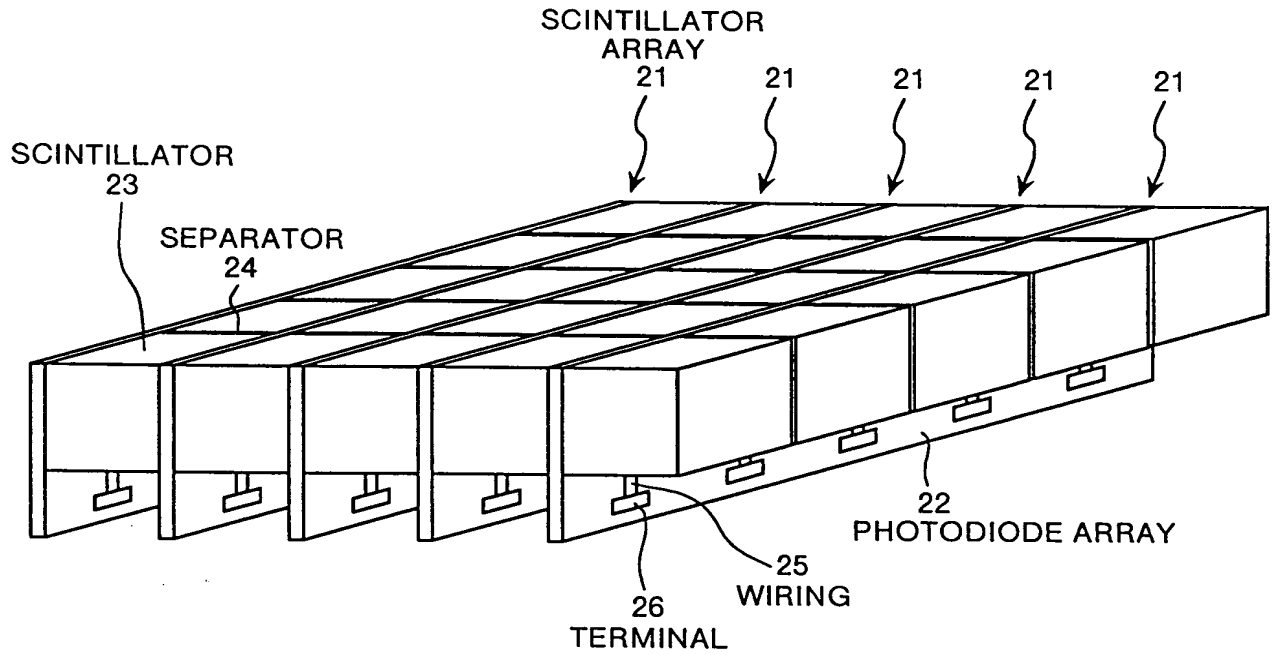


FIG.12

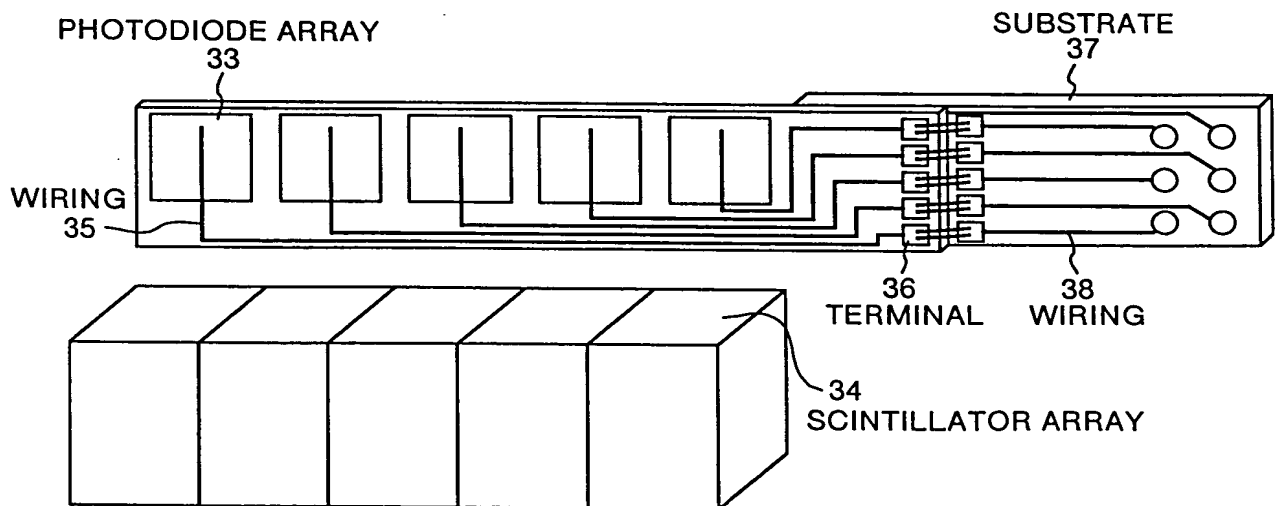


FIG.13

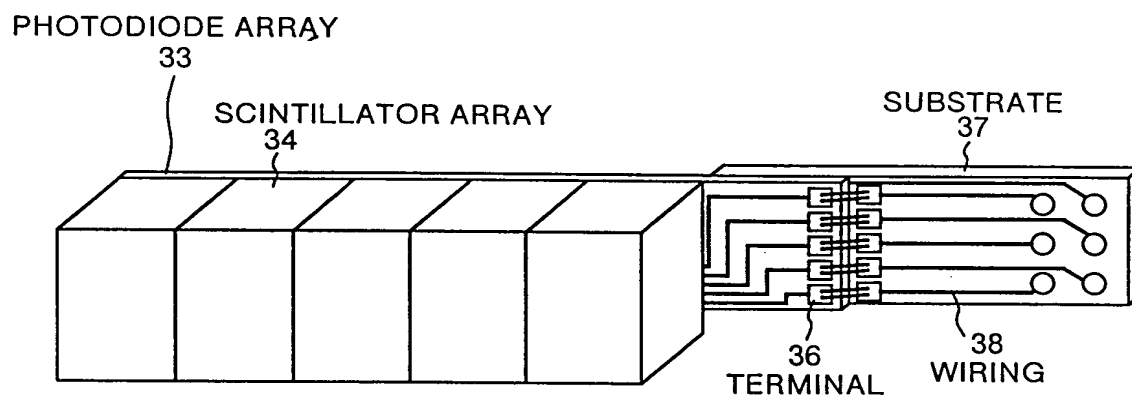


FIG.14

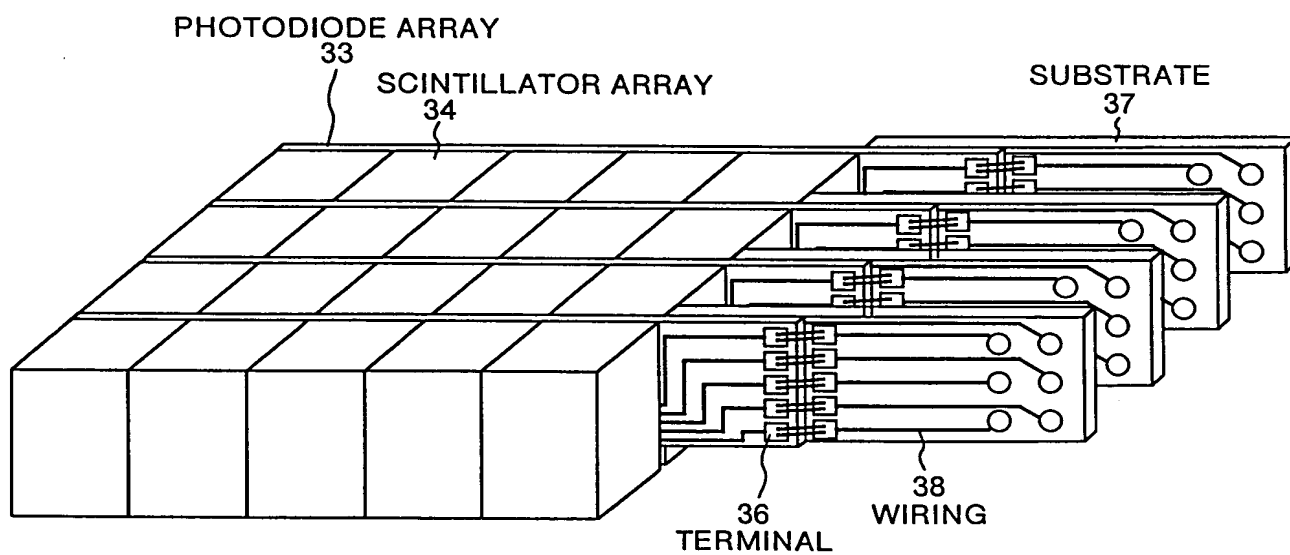


FIG.15A


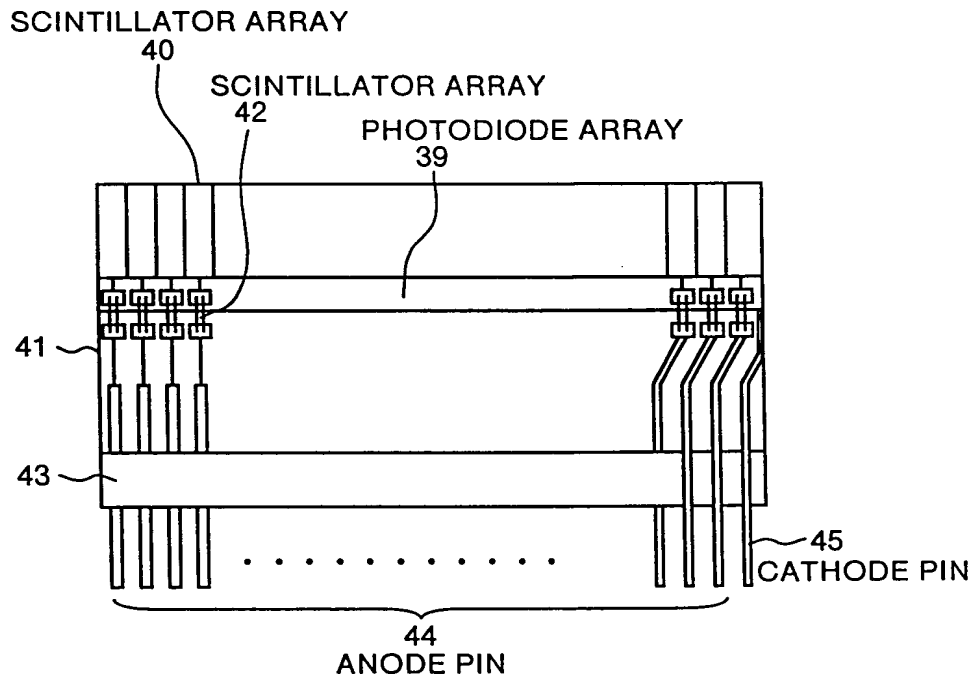


FIG.15B

X-RAY INCIDENT DIRECTION

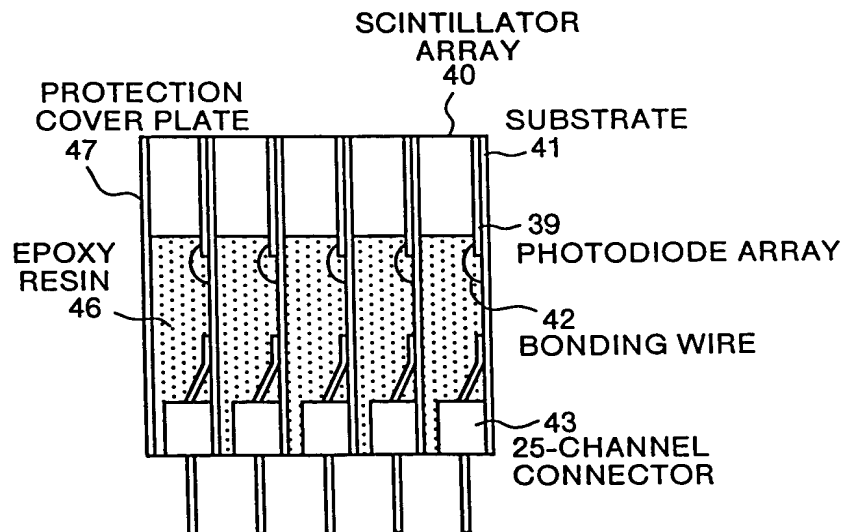

54

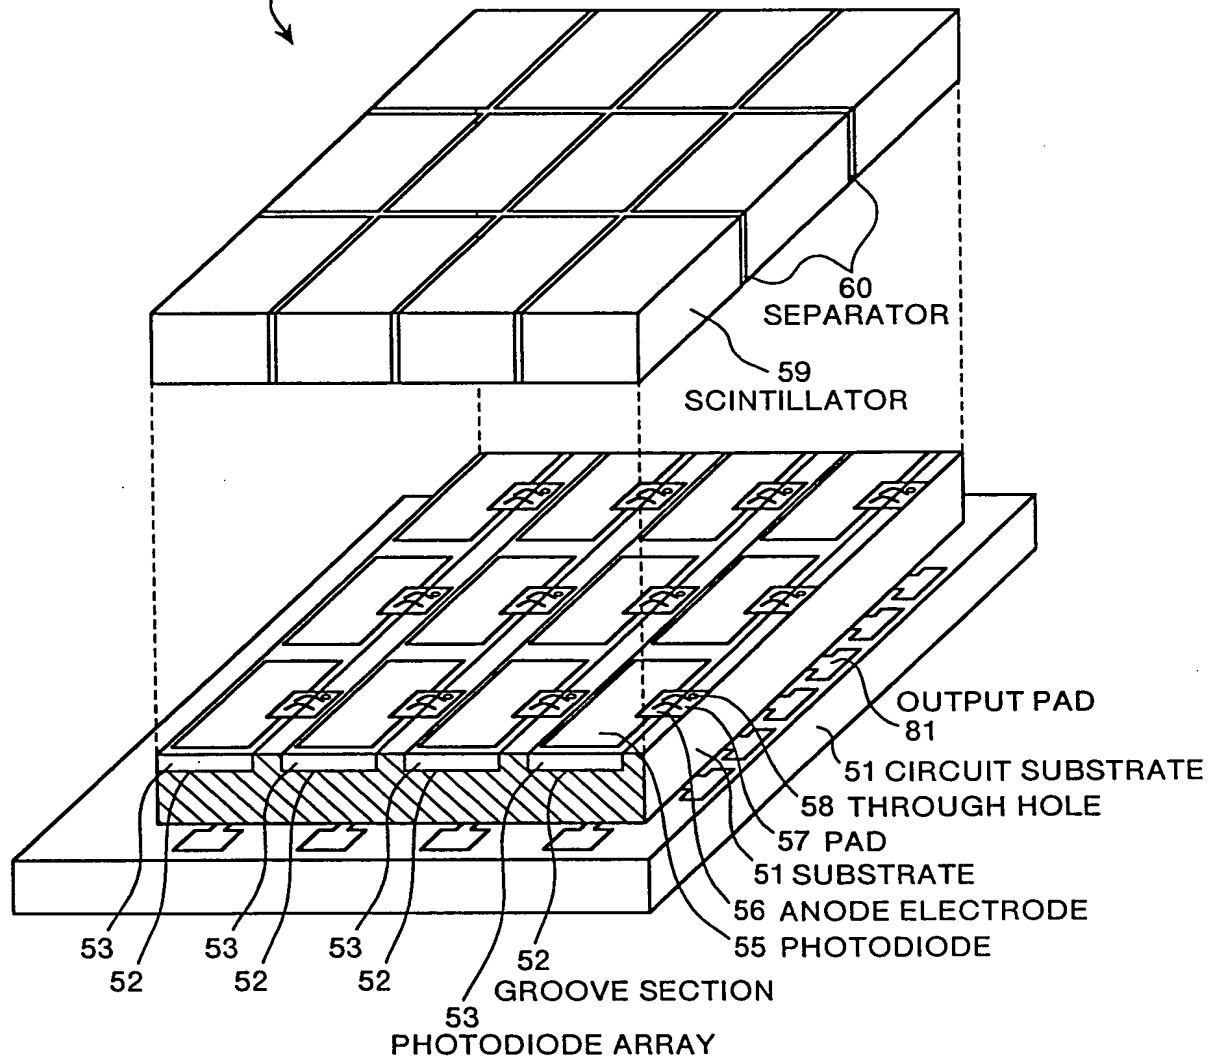


FIG.17

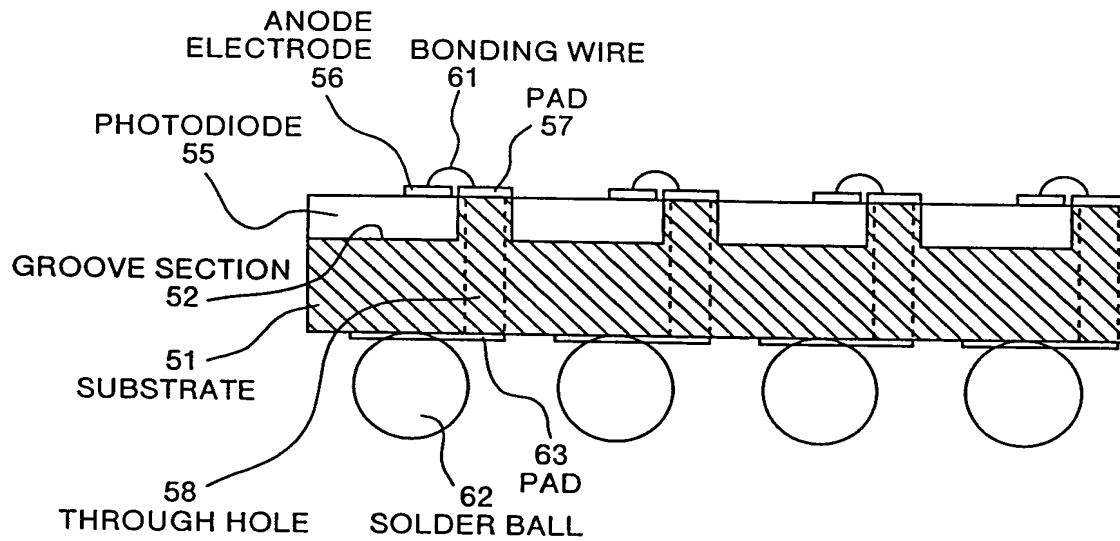


FIG.18

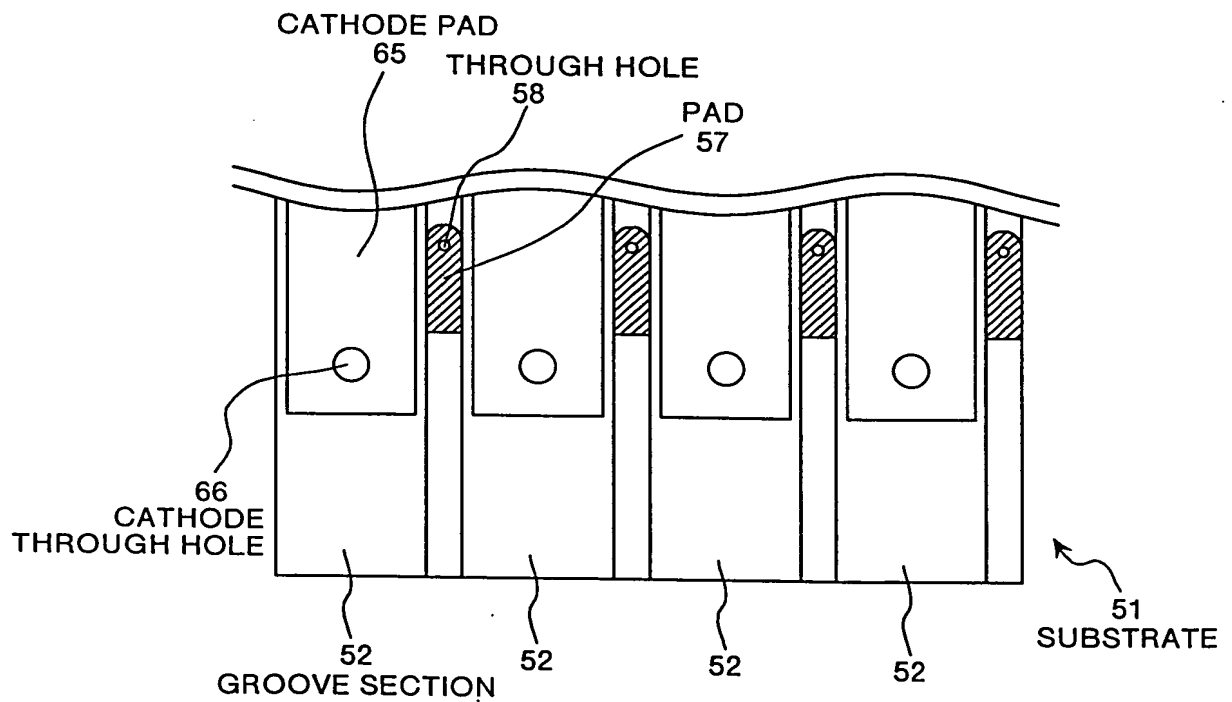


FIG.19

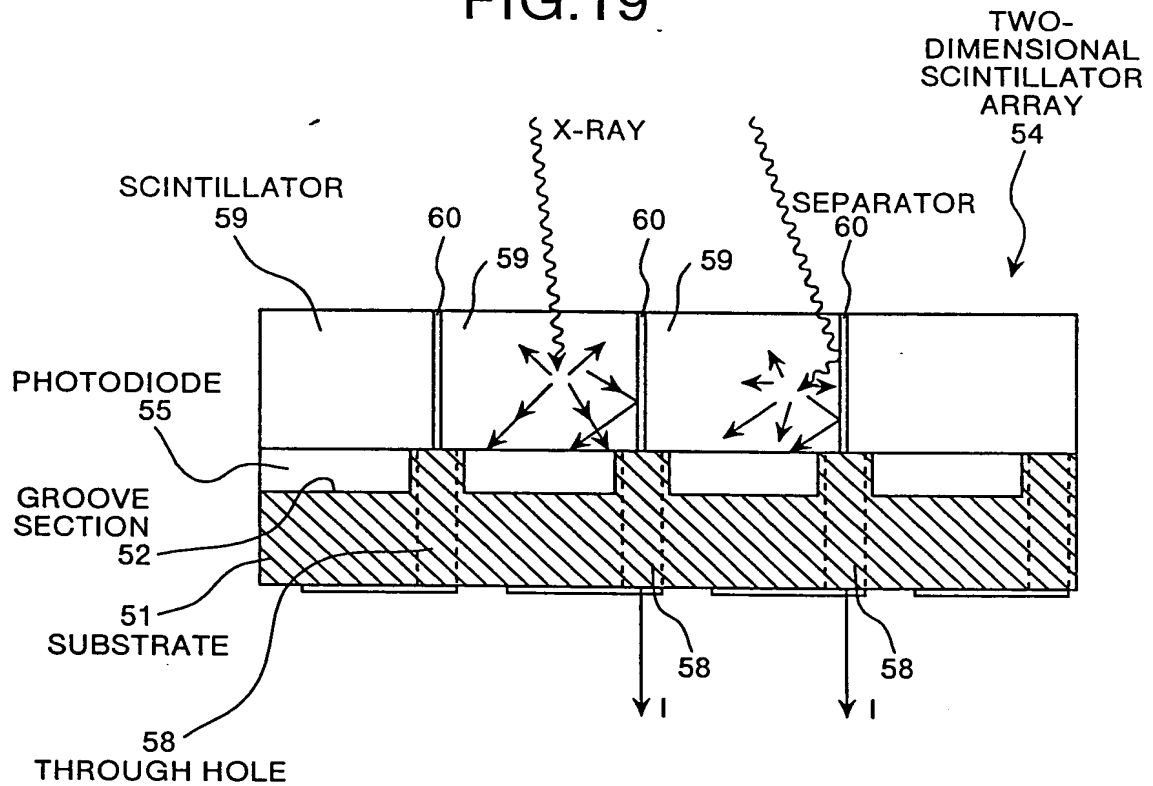


FIG.20

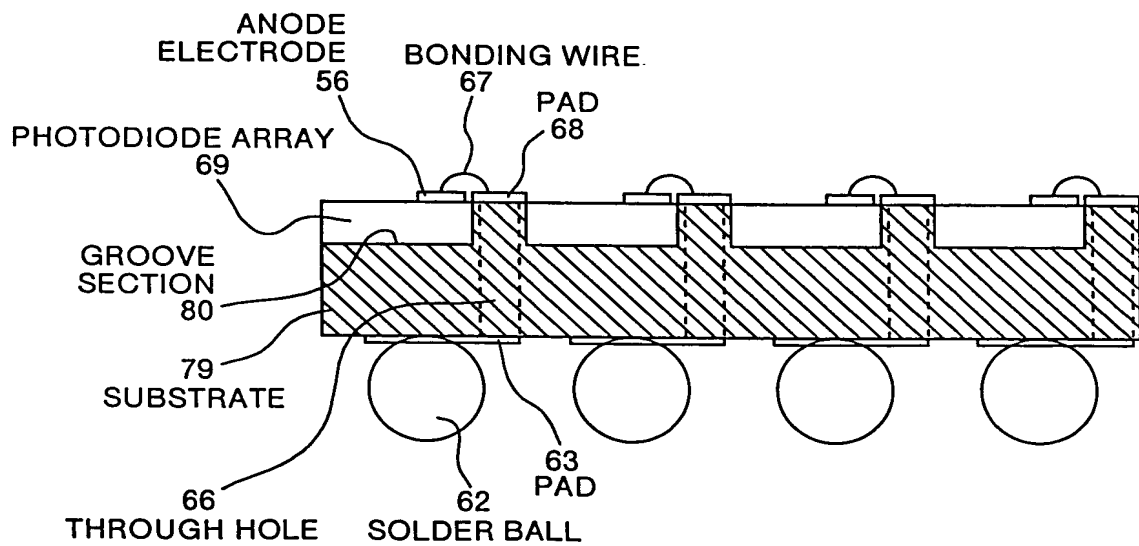


FIG.21

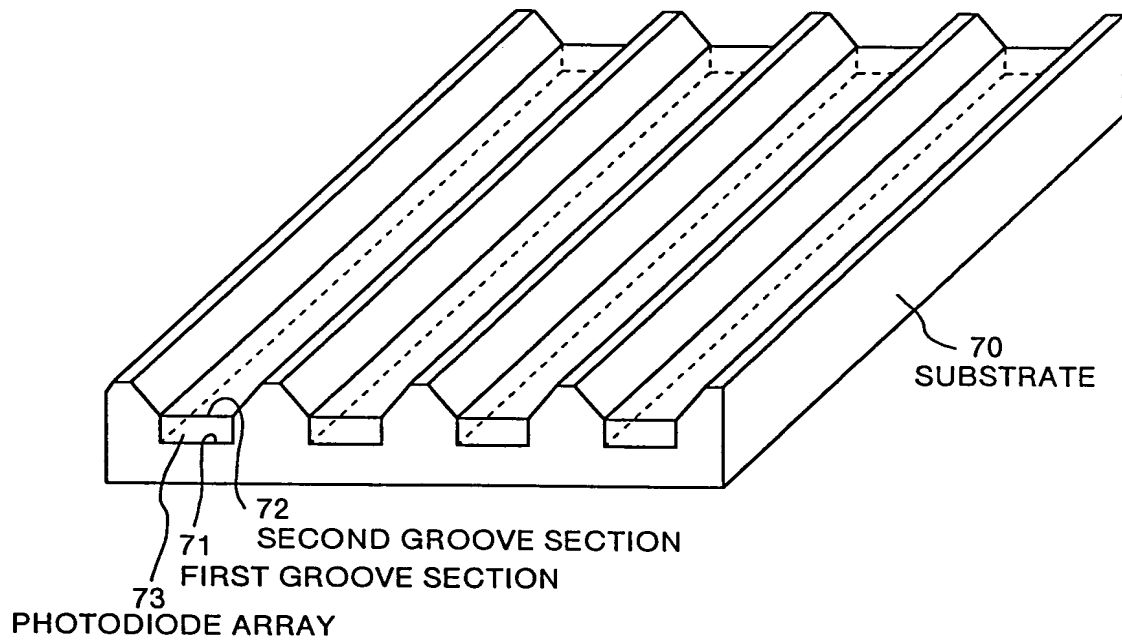


FIG.22

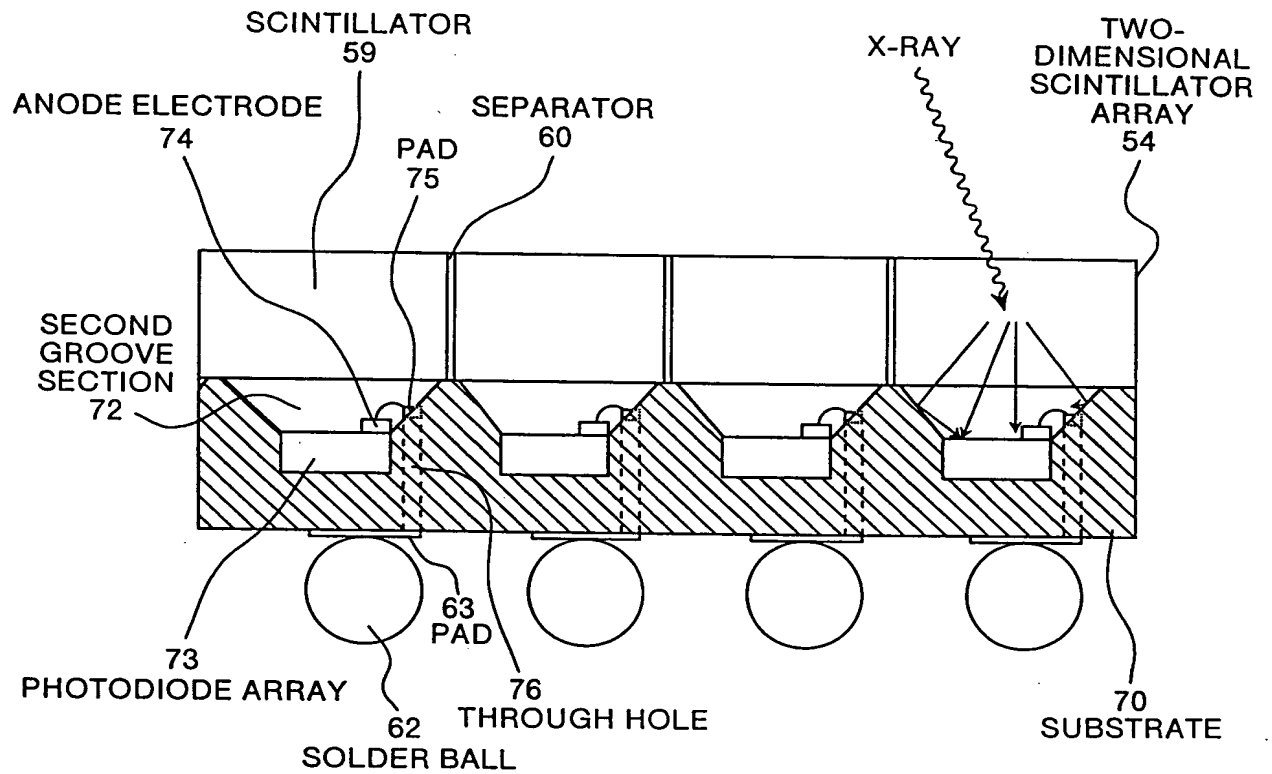




FIG.23

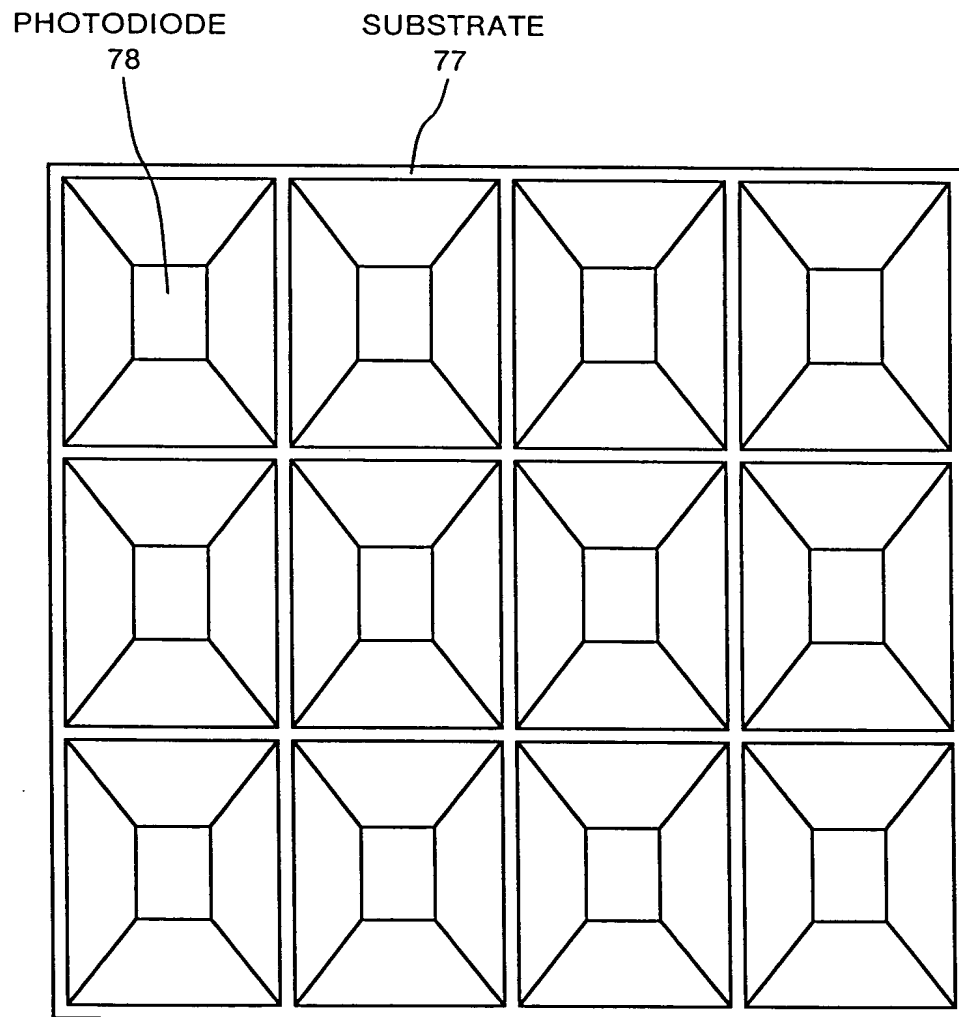


FIG.24A

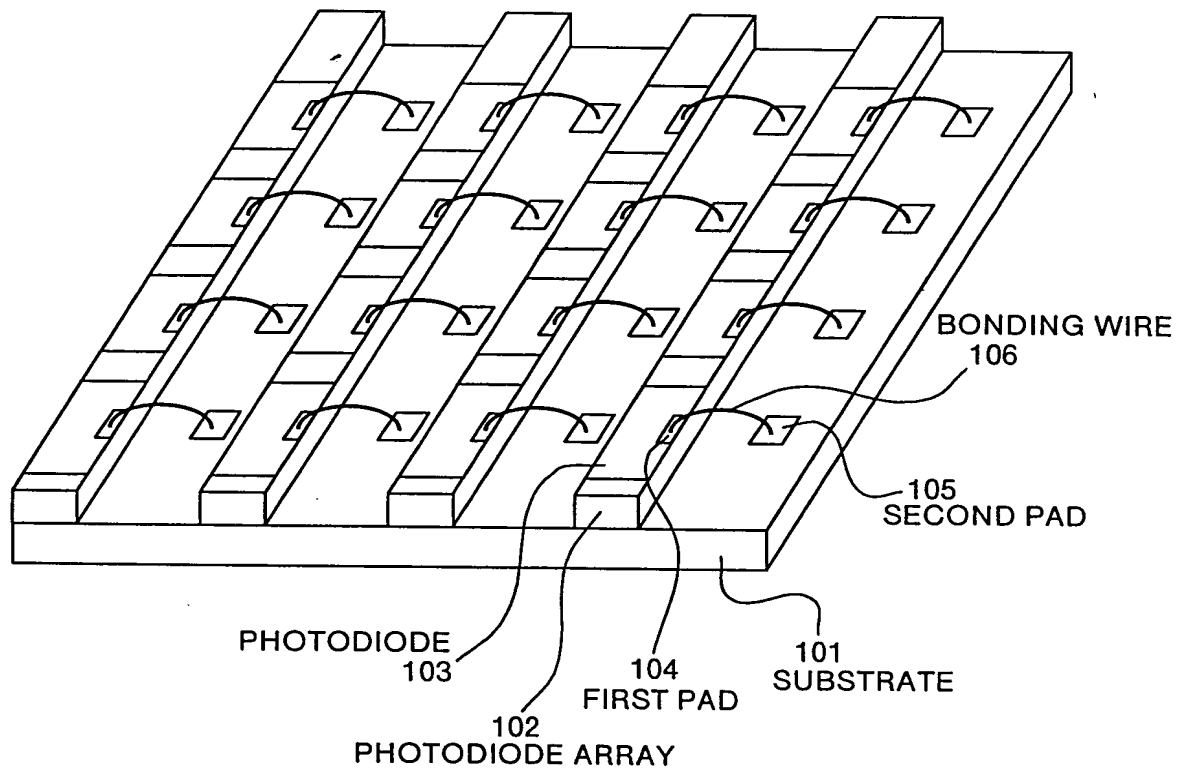


FIG.24B

